



Newtonson4th Ltd

IEC61000 EMC TEST SYSTEMS

- IEC61000-3-2
- IEC61000-3-3
- IEC61000-3-11
- IEC61000-3-12
- IEC61000-4-11
- IEC61000-4-13
- IEC61000-4-14
- IEC61000-4-17
- IEC61000-4-28
- IEC61000-4-29



7949



EMC Test Solutions from the worlds leading IEC61000 test system Manufacturer



N4L EMC Test Systems - The most comprehensive ISO17025 Harmonics and Flicker Calibration coverage in the market

EMC Test Systems

Newtons4th(N4L) design and manufacture a wide range of EMC test systems to meet the needs of modern test laboratories. N4L's high quality instrumentation, accompanied by customized intuitive test software provide highly accurate measurements presented in a clear and concise manner to the user. Sophisticated reporting functions allow the user to rapidly and efficiently export data to excel, producing detailed, professional test reports for end customers.

UKAS ISO17025 Accreditation

N4L PPA55xx series of power analyzers and impedance networks provide fully compliant Harmonics and Flicker test solutions, with direct accreditation available via N4L's internal UKAS ISO17025 calibration laboratory. Certified by NPL (National Physical Laboratory) in the UK, the N4L PPA55xx provides reliable, accurate measurements compliant to the latest test standards (IEC61000-3-2/3 and IEC61000-3-11/12).

In combination with an N4L Impedance Network and a compliant AC Source, you will be equipped to provide fully compliant Harmonics and Flicker measurements.

The level and coverage of accreditation available from the N4L UKAS ISO17025 test laboratory is unrivalled in the industry, the scope of accreditation includes the following;

IEC61000-4-15: Pinst (Sinusoidal and Rectangular Modulation), Pst, Frequency Changes, Distorted Voltage with Multiple Zero Crossings, Harmonics with Sidebands, Phase Jumps, Rectangular Changes with Duty Cycle

IEC61000-4-7: Current Harmonic Amplitude




7949

IEC61000-3-2 / IEC61000-3-12 (Current Harmonics)


The IEC61000-3-2 and IEC61000-3-12 standards refer to the measurement techniques described within the IEC61000-4-7 measurement standard. IEC61000-4-7 details the exact measurement techniques and principles required of an instrumentation manufacturer. The PPA55x1 complies to all aspects of the IEC61000-4-7 standard, thus the PPA55x1 inherently complies to IEC61000-3-2 and IEC61000-3-12. UKAS ISO17025 accreditation is also available from N4L's internal ISO17025 accredited laboratory, this provides the highest level of calibration for an IEC61000-3-2/3-12 harmonics analyzer.

“IECSoft” Software - Harmonic Test Interface

An important aspect of any compliant test system is the HMI(Human Machine Interface), N4L have spent many years developing and improving the IEC61000-3-2/12 user interface which has matured into an intuitive, comprehensive analysis and review mechanism for the test engineer. Features such as real time pass/fail flags, live graphical update of limit levels, data point export for complete test “replay”, as well as a thorough reporting function.

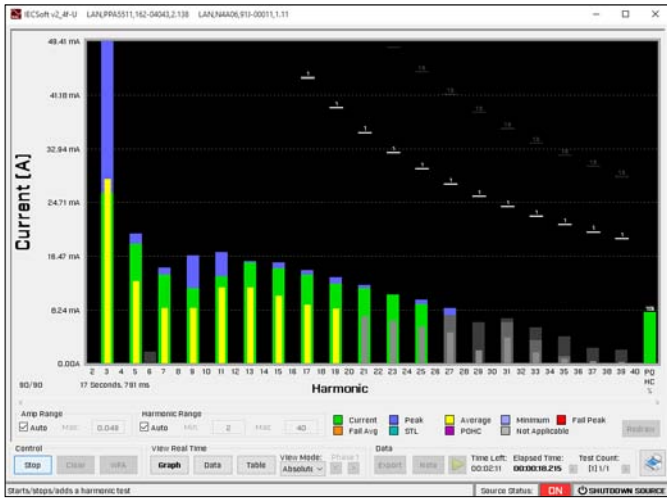

Real time update of colour coded graphical display, including active limit indication

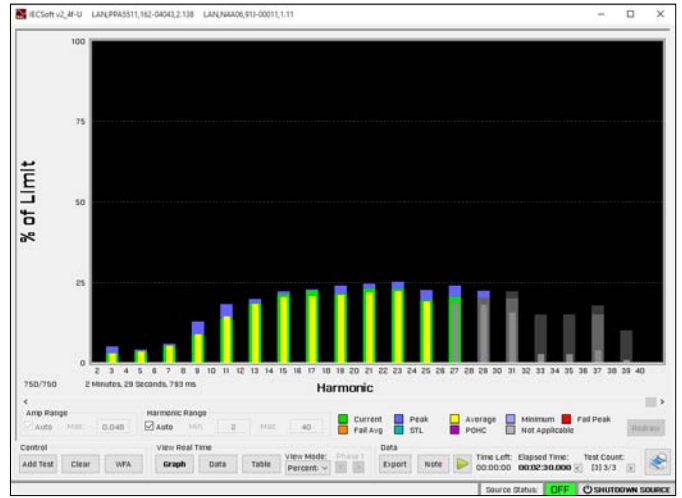

Percentage of limit view normalises each harmonic result to 100% of limit



Individual Harmonics graphed, providing a deeper understanding of DUT behaviour



Unique “Waveform Analysis” mode, providing automated pass/fail result

Harmonics Export Function

The export function integrated into the IECSoft EMC test software suite is a vital aspect of any EMC compliance measurement. IECSoft provides a comprehensive export function directly to excel, this enables the user to edit the report as required to meet internal procedural requirements.

Instrument Details		
Instrument Model	PPA5511	
Instrument Serial	162-04043	
Instrument Firmware	2.138	
Instrument Last Calibrated	02nd February 2015	
Instrument Version	Standard	
Source Model	N4A06	
Source Serial	91J-00011	
Source Frequency	50.000 Hz	
Source Voltage RMS	230.000 V	
Source Settling Time	10 s	
Test Settings		
Class	Class D	
Mode	Measure	
Equipment Under Test		
Brand	Unbranded	
Model	TRW211WS	
Serial	3434908	
Impedance Network ID	91G-11335	
Test Conditions		
User Entered	Measured	
Rated Voltage	230.000 V	230.069 V
Rated Current	4.600 A	992.193 mA
Rated Frequency	50.000 Hz	49.999 Hz
Rated Power	400.000 W	181.809 W
Additional Test Information		
Measured Power Factor	0.6199	
Max Current THD	17.75%	
Max THC	0.0536A	
Max Power	288.051 W	
Max F.Current	1.277 A	
Average F.Current	874.781 mA	
Minimum Current	3A	
Test Duration	2.5 minutes	
Additional Test Details		
Operator	Applications	
Lab Name	N4L	
Location	Leics, UK	
Notes		
Signature		
Results	Phase 1: FAIL - AVERAGE & PEAK	

Harmonic Difference							
Harmonic	Lowest		Highest		Allowance (A)	Limit Difference (A)	Status
	Average (A)	Test #	Average (A)	Test #			
2	0	1	0.000004	3	0	0.000004	PASS
3	0.026425	1	0.026948	3	0.046233	0.000523	PASS
4	0	1	0	3	0	0	PASS
5	0.01827	1	0.018691	3	0.025836	0.000421	PASS
6	0	3	0.000014	1	0	0.000014	PASS
7	0.013636	1	0.014261	3	0.013598	0.000625	PASS
8	0	1	0	3	0	0	PASS
9	0.01171	1	0.012132	3	0.006799	0.000422	PASS
10	0	1	0.000001	3	0	0.000001	PASS
11	0.01351	1	0.013681	3	0.004759	0.000171	PASS
12	0	1	0	3	0	0	PASS
13	0.014495	1	0.014659	3	0.004027	0.000164	PASS
14	0	1	0	3	0	0	PASS
15	0.013833	1	0.014275	3	0.00349	0.000442	PASS
16	0	1	0	3	0	0	PASS
17	0.012738	3	0.012796	1	0.00308	0.000058	PASS
18	0	1	0	3	0	0	PASS
19	0.011593	3	0.011857	1	0.002755	0.000264	PASS
20	0	1	0	3	0	0	PASS
21	0.010707	1	0.010911	3	0.002493	0.000204	PASS
22	0	1	0	3	0	0	PASS
23	0.009389	1	0.010102	3	0.002276	0.000713	PASS
24	0.00005	3	0.000069	1	0	0.00002	PASS
25	0.008008	3	0.008477	1	0.002094	0.000469	PASS
26	0.000023	3	0.000051	1	0	0.000028	PASS
27	0.006877	1	0.007284	3	0.001939	0.000407	PASS
28	0	1	0	3	0	0	PASS
29	0.003537	1	0.006486	3	0.001805	0.002949	FAIL
30	0	1	0	3	0	0	PASS
31	0.00464	1	0.005309	3	0.001689	0.00067	PASS
32	0	3	0.000001	1	0	0.000001	PASS
33	0.000872	3	0.002616	1	0.001586	0.001744	FAIL
34	0	1	0	3	0	0	PASS
35	0.000607	1	0.000843	3	0.001496	0.000236	PASS
36	0	1	0	3	0	0	PASS
37	0.000334	1	0.001104	3	0.001415	0.00077	PASS
38	0	1	0	3	0	0	PASS
39	0.000231	3	0.000275	1	0.001342	0.000044	PASS
40	0	1	0	3	0	0	PASS

Key:
 Allowance Maximum Difference allowed in Amps
 Good The difference is less than 50% of the allowance
 OK The difference is between 50% of the allowance and 75% of the allowance
 Poor The difference is between 75% of the allowance and 100% of the allowance
 Fail The difference has exceeded the allowance


IEC61000-3-3 / IEC61000-3-11 (Flicker IEC61000-4-15)

N4L provide complaint measurements to the latest test protocols/limits specified within IEC61000-3-3 and IEC61000-3-11. The PPA551 Precision Power Analyzer complies fully with IEC61000-4-15 which dictates both the hardware and firmware requirements for compliance to IEC61000-3-3/11. N4L are currently the only Flickermeter manufacturer in the world* to offer complete coverage of the IEC61000-4-15 standard with ISO17025 accreditation. This optional ISO17025 calibration procedure is performed within N4L's ISO17025 UKAS calibration laboratory and covers all aspects of the IEC Flicker test standards.


"IECSoft" Software Flicker Test Interface

IECSoft's Flicker measurement mode incorporates an intuitive step by step style setup procedure, guiding the user through the test configuration. Remote control of the N4L N4A AC Power Source is handled automatically by IECSoft, test procedures include selection of d[t] parameters and calculation of Z_{test} if necessary. Pinst, IFS, PST, PLT, D, Dmax, Dc and Tmax are also updated during any test.

* According to N4L research 2014

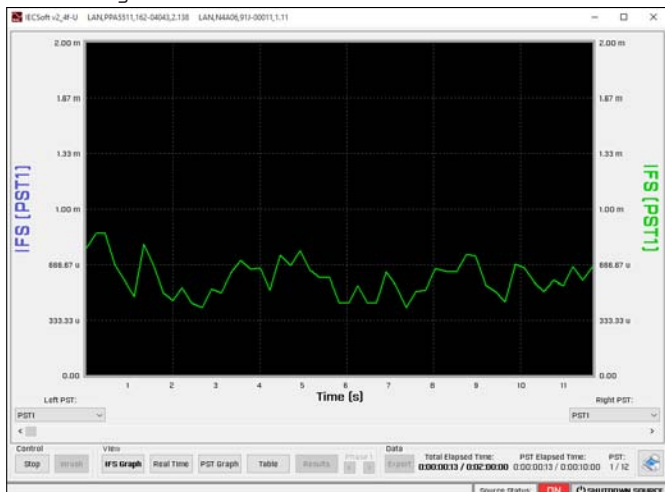


IFS recorded real time, for in depth post test analysis

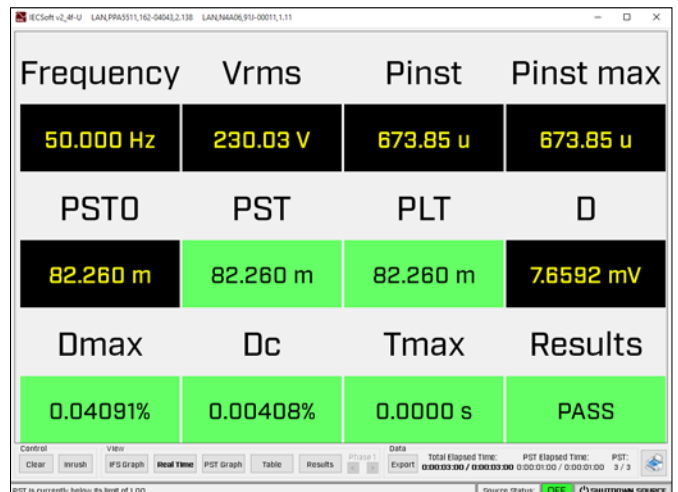

Real time display indicating current test status

Phase	Time	Frequency	Vrms [V]	Power [W]	PST	PLT	D	Dmax [s]	Dc [s]	Time [s]		
135	-00:00:32.184	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0047	0.0335	0.0050	0.0000
136	-00:00:32.401	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0017	0.0335	0.0050	0.0000
137	-00:00:32.618	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0025	0.0335	0.0050	0.0000
138	-00:00:32.835	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0107	0.0335	0.0050	0.0000
139	-00:00:33.052	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0148	0.0335	0.0050	0.0000
140	-00:00:33.269	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0184	0.0335	0.0050	0.0000
141	-00:00:33.486	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0123	0.0335	0.0050	0.0000
142	-00:00:33.703	50.0000	229.7400	0.0010	0.0014	0.0063	0.0000	0.0000	0.0148	0.0335	0.0050	0.0000
143	-00:00:33.920	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0175	0.0335	0.0050	0.0000
144	-00:00:34.137	50.0000	229.7400	0.0008	0.0014	0.0063	0.0000	0.0000	0.0100	0.0335	0.0050	0.0000
145	-00:00:34.354	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0096	0.0335	0.0050	0.0000
146	-00:00:34.571	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0029	0.0335	0.0050	0.0000
147	-00:00:34.788	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0182	0.0335	0.0050	0.0000
148	-00:00:35.005	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0024	0.0335	0.0050	0.0000
149	-00:00:35.222	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0033	0.0335	0.0050	0.0000
150	-00:00:35.439	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0148	0.0335	0.0050	0.0000
151	-00:00:35.656	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0110	0.0335	0.0050	0.0000
152	-00:00:35.873	50.0000	229.7400	0.0008	0.0014	0.0063	0.0000	0.0000	0.0237	0.0335	0.0050	0.0000
153	-00:00:36.090	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0116	0.0335	0.0050	0.0000
154	-00:00:36.307	50.0000	229.7400	0.0010	0.0014	0.0063	0.0000	0.0000	0.0141	0.0335	0.0050	0.0000
155	-00:00:36.524	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0079	0.0335	0.0050	0.0000
156	-00:00:36.741	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0064	0.0335	0.0050	0.0000
157	-00:00:36.958	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0073	0.0335	0.0050	0.0000
158	-00:00:37.175	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0027	0.0335	0.0050	0.0000
159	-00:00:37.392	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0013	0.0335	0.0050	0.0000
160	-00:00:37.609	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0013	0.0335	0.0050	0.0000
161	-00:00:37.826	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0144	0.0335	0.0050	0.0000
162	-00:00:38.043	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0040	0.0335	0.0050	0.0000
163	-00:00:38.260	50.0000	229.7400	0.0005	0.0014	0.0063	0.0000	0.0000	0.0019	0.0335	0.0050	0.0000
164	-00:00:38.477	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0006	0.0335	0.0050	0.0000
165	-00:00:38.694	50.0000	229.7400	0.0006	0.0014	0.0063	0.0000	0.0000	0.0038	0.0335	0.0050	0.0000
166	-00:00:38.911	50.0000	229.7400	0.0007	0.0014	0.0063	0.0000	0.0000	0.0070	0.0335	0.0050	0.0000
167	-00:00:39.128	50.0000	229.7500	0.0006	0.0014	0.0063	0.0000	0.0000	0.0033	0.0335	0.0050	0.0000

Every data return is recorded and saved within the IECSoft software package

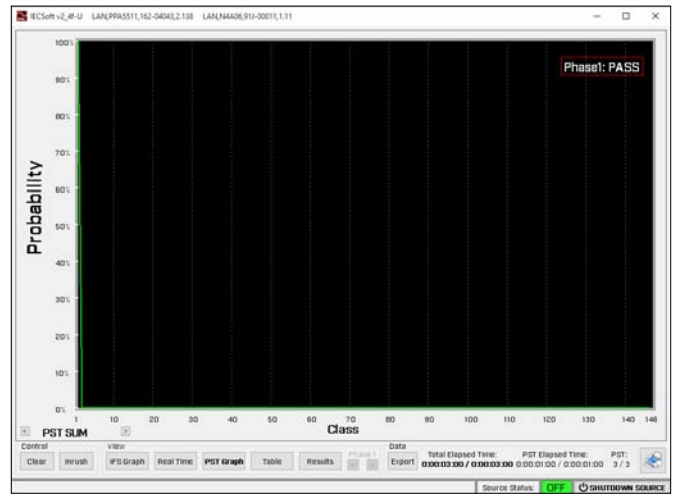

Classifier Probability Graph

Inrush Testing [dmax]

For products utilising manual switching as a method of initiating and ending operation, a “dmax” test as the “Inrush test” is required. This involves a succession of 24 switching events that are recorded and the arithmetic mean (excluding the highest and lowest dmax values) is calculated. An intuitive user interface has been developed for this task which guides the test engineer through the process and provides prompts to perform the switching event. Statistical analysis is also automated within the software, removing this burden from the user. This results in reduced test times and eliminates the risk of a mathematical error.

Wait command indicated by the “Inrush test” user interface

“Start OUT” Command to prompt user to operate manual switch

Flicker Export Function

The flicker export function exports all recorded data including DUT test data and flicker results, export options include the ability to lock the exported spreadsheet as well as formatting the report into a single or multiple worksheet. The user also has the ability to import their own company logo, which is exported within the final report.

Export user interface


Instrument Details		
Instrument Model	PPA511	
Instrument Serial	162-04043	
Instrument Firmware	2.138	
Instrument Last Calibrated	02nd February 2015	
Instrument Version	Standard	
Source Model	N4A06	
Source Serial	911-00011	
Source Frequency	50.000 Hz	
Source Voltage RMS	230.000 V	
Source Settling time	10 s	
Test Settings		
Class	Voltage	
Mode	Normal - 4%	
Minimum Current	10A	
PST	1.00 minutes	
PLT	3 PSTs	
Equipment Under Test		
Brand	Unbranded	
Model	TRW211WS	
Serial	3434908	
Impedance Network ID	91G-11335	
Test Conditions		
User Entered		Measured
Rated Voltage	230.000 V	229.726 V
Rated Current	4.500 A	N/A
Rated Frequency	50.000 Hz	50.000 Hz
Rated Power	400.000 W	N/A
D max	0.0428% (Limit: 4%)	
T max	0.0000 s (Limit: 0.5 s)	
DC max	0.0008% (Limit: 3.3%)	
Additional Test Details		
Operator	Applications	
Lab Name	N4L	
Location	Leics, UK	
Notes		
Signature		
Results	Phase1: PASS	

IEC61000-4-15 - Flicker Simulation


N4A power sources are able to simulate flicker waveforms in order to test flickermeters for correct operation. This mode can also be used to create an environment in which products are tested for susceptibility against flicker on the supply line, this is useful as voltage modulations on the supply line can cause instability within input regulation circuitry.

IEC61000-4-11 - Voltage Dips, Short Interruptions and Voltage Variations

IEC61000-4-11 defines test protocols and measurement techniques for electrical and electronic equipment connected to low-voltage supply networks. IECSoft provides an easy to configure user interface, in which a number of product configurations can be added to the test sequences. Covering all classes, including class "X" - the software offers the flexibility required for product committees to define a wide range of test levels.

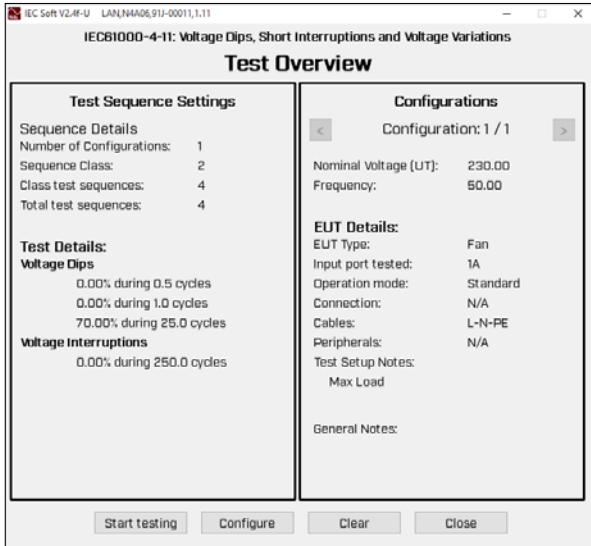


Test overview interface - Detailing the class, number of sequences and test details

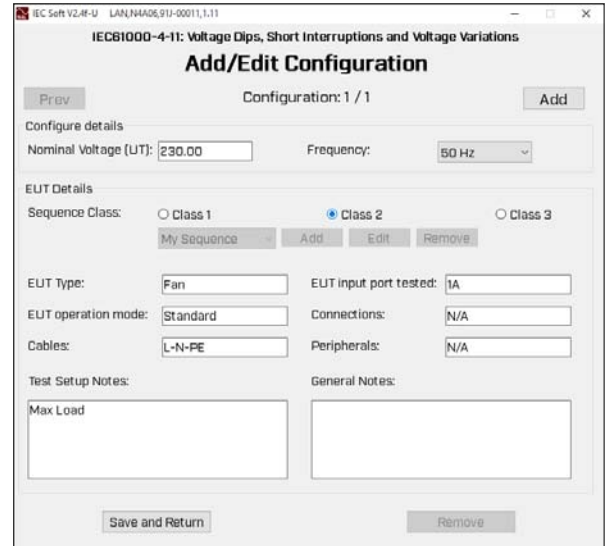

Configuration interface - Select class, product details and nominal voltage/frequency



Test sequence - AC Source ON awaiting manual initiation of test sequence.

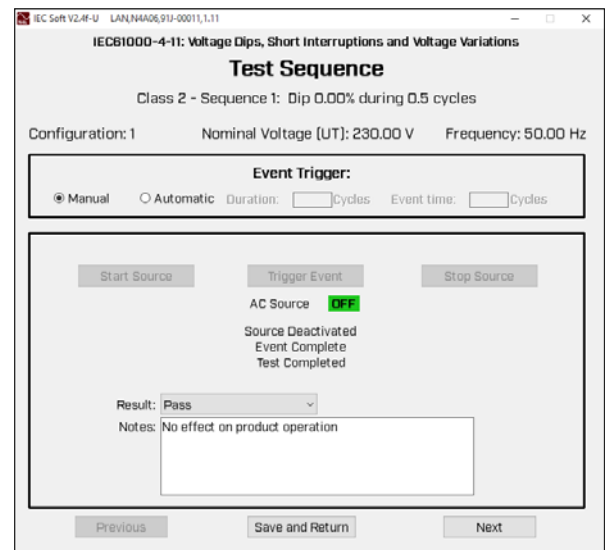

Test Complete - DUT passed

Source Details	
Source Model	N4A06
Source Serial	91J-00011
Source Firmware	1.11
Equipment Under Test	
Brand	Unbranded
Model	TRW211WS
Serial	3434908
Impedance Network ID	91G-11335
Rated Voltage	230 V
Rated Current	4.6A
Rated Frequency	50-60 Hz
Rated Power	400W
Additional Test Details	
Operator	Applications
Lab Name	N4L
Location	Leics, UK
Notes	
Signature	

Test report for IEC61000-4-11

Instrument Details	
Source Model	N4A06
Source Serial	91J-00011
Source Firmware	1.11
Equipment Under Test	
Brand	Unbranded
Model	TRW211WS
Serial	3434908
Equipment Under Test	
EUT Type	Fan
Input Port	1A
Operating Mode	Standard
Connections	N/A
Cables	L-N-PE
Peripherals	N/A
Setup Notes	Max Load
General Notes	
Configuration Settings	
Nominal Voltage (UT)	230.00 V
Frequency	50.00 Hz
Sequence Class	2
Test Results 1/4	
Test Type	Dip
Test Level	0.00%
Duration in cycles	0.5
Test Notes	No effect on product operation
Test Results	Pass


IEC61000-4-11 Test Details

IEC61000-4-13 - Harmonic and Interharmonic Susceptibility


As mains supply lines can suffer from harmonic and interharmonic interference, IEC61000-4-13 defines the harmonic and interharmonic levels upon which products must be tested. IECSoft provides a simple user interface to create test programmes for each class of product.




IEC61000-4-13 EUT Setup interface including class selection

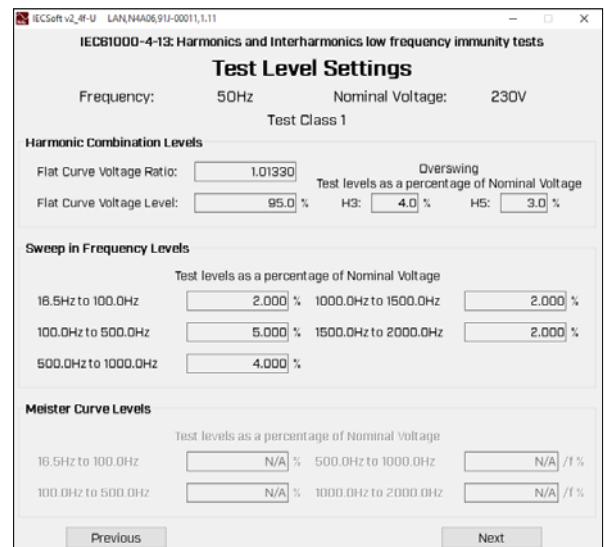

Test programme details including harmonic combination and frequency sweep

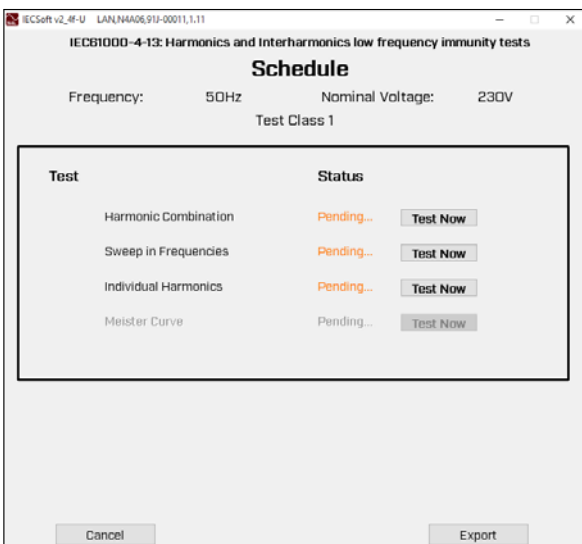


IEC61000-4-13 Test Schedule

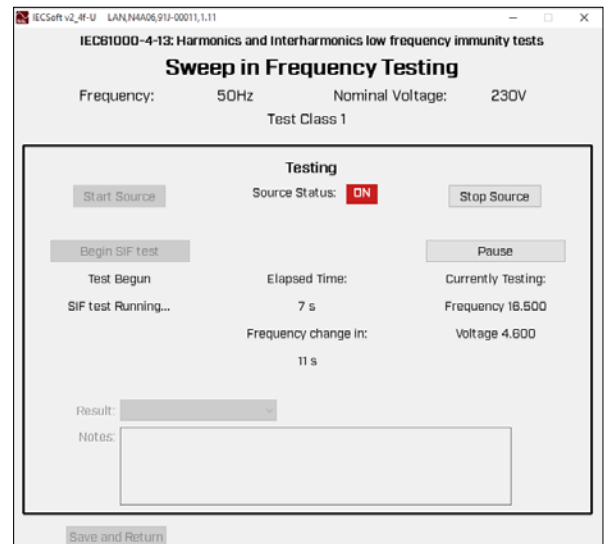

Sweep in Frequency test in progress

Power Source Schematic

N4A Advanced Power Amplifiers feature proprietary noise suppression analogue electronics known as "6 leg modulation" topology which produces an output waveform during high loads with less than 0.1% THD. This level of distortion has only previously been possible with linear power sources.

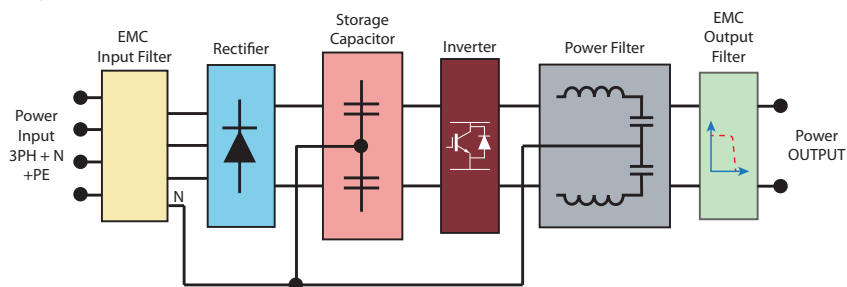

IEC61000 EMC TEST SYSTEM SPECIFICATION:

PPA55x1 Harmonics and Flicker Analyzer


PPA55x1 Harmonics and Flicker Analyzer	
Bandwidth	
	DC, 10mHz ~ 1MHz - PPA55x1 - Low Impedance Shunt (50Arms)
IEC61000 Voltage Input	
Range	300mVpk ~ 3000Vpk(1000Vrms) in 9 ranges
	0.01% Rdg+0.038% Rng+(0.004%×kHz)+5mV
Range	300μVpk ~ 3Vpk in 9 ranges [BNC connector 3Vpk max input]
	0.01%Rdg+0.038%Rng+(0.004%×kHz)+3μV
IEC61000-3-2 Compliant Current Input, including Harmonic Accuracy	
Low Impedance (Fully Compliant) 3mΩ Max 50Arms	100mApk ~ 1000A(50Arms)
	0.01% Rdg+0.038% Rng+(0.004%×kHz)+ 900μA
External input (External shunt Current sensor)	BNC Connector (Max input 3Vpk)
	300μVpk ~ 3Vpk in 9 ranges
	0.01% Rdg+0.038% Rng+(0.004%×kHz)+ 3μV
Phase Accuracy	
	0.005deg+(0.01deg×kHz) [PPA5500-LC(10Arms), PPA5500(30Arms)]
	0.01deg+(0.02deg×kHz) [PPA5500-HC(50Arms)]
IEC61000-3-3 + IEC61000-3-11 Flicker Accuracy	
Pst	3%
Plt	3%
Pinst	5%
d(c), d(max), d(t)	3%
IEC61000-3-2 + IEC61000-3-12 Harmonics Accuracy	
	0.1% of rms current
Power Accuracy	
	[0.03%+0.03%/pf+(0.01%×kHz)/pf] Rdg+0.03%VA Rng
40-400Hz	[0.03%+0.03%/pf+(0.01%×kHz)/pf] Rdg+0.02%VA Rng
General	
Crest Factor	20(Voltage and Current)
Sample Rate	2.2Ms/s on all channels, No-Gap
IEC Modes	IEC61000 Harmonics and Flicker (PPA5500), IEC62301 Standby Power
Application Modes	PWM Motor Drive, Ballast, Inrush, Power Transformer, Standby Power, Fluctuating Harmonics, Flicker Meter
CMRR - Common Mode Rejection Ratio	
	250V @ 50Hz - ≥ 1mA (150dB)
	100V @ 100kHz - ≥ 3mA (130dB)

Measurement Parameters	
	W, VA, Var, pf, V & A - rms, rectified mean, AC, DC, Peak, Surge, Crest Factor, Form Factor, Star to Delta Voltage
	Frequency (Hz), Phase (deg), Fundamentals, Impedance
	Harmonics, THD, TIF, THF, TRD, TDD
	Integrated Values, Datalog, Sum and Neutral values
Datalog - Up to 4 user selectable measurement functions (60 with optional PC software)	
Datalog Window	No-Gap analysis, Minimum window 2ms
Memory	10M records into flash RAM (Non-Volatile)

Communication Ports	
RS232	Baud rate up to 38.4kbps, RTS/CTS flow control
LAN	10/100 Base-T Ethernet auto sensing
GPIB	IEEE488.2 compatible
USB	USB 2.0 and 1.1 compatible
Analogue Output	Bipolar ±10V(BNC)
Speed Input	BNC Bipolar±10V or Pulse count 1Hz to 1MHz 0.01% Rdg
Torque	BNC Bipolar±10V or Pulse count 1Hz to 1MHz 0.01% Rdg
Sync	4 ~ 6 Phase measurement (Master/Slave)
Extension	4 ~ 6 Phase (Master/Slave) + Auxiliary
Standard Accessories	
Leads	Power, RS232, USB, GPIB
Connection Cables	36A 1.5m long 4mm stackable terminals 1x red, 1x yellow and 2x black per phase (1x red, 1x black with HC version)
Connection Clips	4mm terminated alligator clips - 1x red, 1x yellow and 2x black per phase (1x red and 1x black per phase with PPA5500-HC version)
CD-ROM	IECSOft, CommView2 (RS232/USB/LAN), Command line, Script based communication software
Documents	User manual, Communications manual, Calibration certificate, Quick start guide
Mechanical/Environmental	
Display	320×240 dot full colour TFT, White LED Backlit
Dimensions	130H×400W×315D mm excluding feet
Weight	5.4kg(1 Phase), 6kg(3 Phase)
Safety Isolation	1000Vrms or DC(CATII), 600Vrms or DC(CATIII)
Power supply	90 ~ 265Vrms, 50 ~ 60Hz, 40VAmax

IMPEDANCE NETWORK SPECIFICATION

IMP161/3(16Arms) , IMP321/3(32Arms) and IMP753(75Arms) models available	
IMP161/3	Fully Compliant to IEC61000-3-3
IMP321/3 & IMP753	Fully Compliant to IEC61000-3-11
Impedance Specification	
	$R_s = 0.24\Omega$ $jX_s = 0.15\Omega$ @ 50Hz $R_n = 0.16\Omega$ $jX_n = 0.10\Omega$ @ 50Hz
Current Rating	
IMP16x	16Arms per phase
IMP753	75Arms per phase

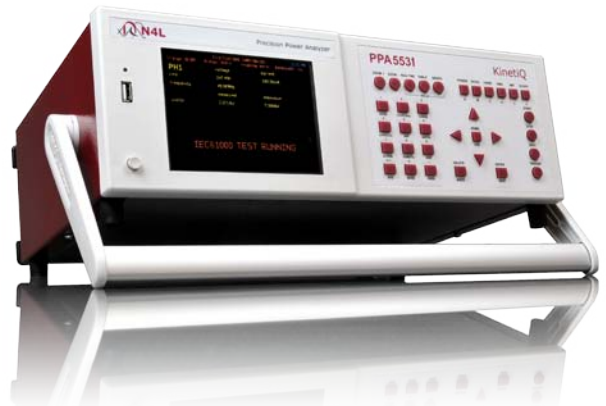


PPA5531 Harmonics and Flicker Analyzer

AC POWER SOURCE SPECIFICATION

	N4A03 (1 Phase)	N4A06 (1 Phase)	N4A18 (3 Phase)	N4A30 (3 Phase)	N4A67 (3 Phase)
Nominal Output Power	3,000VA	6,000VA	18,000VA	30,000VA	67,500kVA
Compliant Standards	IEC61000-3-2:2014 (Single Phase) IEC61000-3-3:2013 (Single Phase) IEC61000-4-11:2004 (Single Phase) IEC61000-4-13:2009 (Single Phase) IEC61000-4-14:1999 (Single Phase) IEC61000-4-17:2009 (Single Phase) IEC61000-4-28:2000 (Single Phase) †IEC61000-4-29:2001 (Single Phase)		IEC61000-3-2:2014 (Single/Three Phase) IEC61000-3-3:2013 (Single/Three Phase) IEC61000-3-12:2005 (Single/Three Phase) IEC61000-3-11:2000 (Single/Three Phase) IEC61000-4-11:2004 (Single/Three Phase) IEC61000-4-13:2009 (Single/Three Phase) IEC61000-4-14:1999 (Single/Three Phase) IEC61000-4-17:2009 (Single Phase) IEC61000-4-28:2000 (Single/Three Phase) †IEC61000-4-29:2001 (Single Phase)		
Output					
Output Voltage (AC)	0-300Vrms				
Output Voltage (DC)	0-425V DC				
Maximum Continuous Output Power (AC)	3000VA	6000VA	18,000VA	30,000VA	67,500VA
Maximum Inrush (3 Second) Output Power (DC)	6000VA	12000VA	36,000VA	60,000VA	90,000VA
Maximum Output Current (Continuous)	10Arms	20Arms	20Arms (Per Phase)	32Arms (Per Phase)	75Arms (Per Phase)
Maximum Output Current (Inrush)	20Arms	40Arms	40Arms (Per Phase)	64Arms (Per Phase)	100Arms (Per Phase)
Output Frequency	DC - 1kHz	DC - 1kHz	DC - 1kHz	DC - 1kHz	DC - 1kHz
Min Slew Rate	3V/us	3V/us	3V/us	3V/us	3V/us
Output Voltage Stability	Better than 0.1%				
Output Voltage Accuracy	Better than 0.5%				
THD	Better than 0.3%▲				
Output Noise	<500mVrms				
Recovery Time of Output Waveform	Better than 50us				
Max Compensated drop on wires (w.r.t voltage setting)	5%				
Recovery Time of Drop on Wires	Less than 200ms				
Maximum Crest Factor	[Inrush I _{max} x 1.41]/RMS Load Current				
General					
Dimensions	281mm x 471mm x 513mm		1785mm x 930mm x 755mm	1785mm x 930mm x 755mm	1800mm x 1200mm x 800mm
Weight	30kg	45kg	740kg		1300kg
Input Voltage	220V AC +/- 10% 1PH 230V AC +/- 10% 1PH	380V AC +/- 10% 3PH 400V AC +/- 10% 3PH 415V AC +/- 10% 3PH			
Input Frequency	45-65Hz				
Operating Temperature	0-35degC				
Input Current	24Arms	16Arms Phase / 27A Neutral	60A continuous 120A inrush / Phase	80A continuous 160A inrush / Phase	160A continuous 220A inrush / Phase
Efficiency	Better than 80%				

† Pre-compliant due to rise/fall time of generator

▲At Nominal Voltage with Linear Load

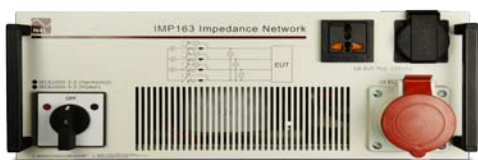


IMP163 3 Phase 16Arms/Phase Impedance Network

Overview of IEC61000 Test Systems

IEC61000 Test Systems			
System Configuration			
Overall System Description	Single Phase 16A IEC61000 EMC Test System	Single+Three Phase 16A IEC61000 EMC Test System	Single+Three Phase up to 75A IEC61000 EMC Test System
Power Source	N4A06	N4A18	N4A67
Harmonics and Flicker Analyzer	PPA5511 Combined Harmonics and Flicker + Power Analyzer	PPA5531 Combined Harmonics and Flicker + Power Analyzer	PPA5531 Combined Harmonics and Flicker + Power Analyzer
Optional Impedance Network (For compliant Flicker testing)	IMP161	IMP163	IMP753
Standards (Limits)	IEC61000-3-2:2014 (Single Phase) IEC61000-3-3:2013 (Single Phase) IEC61000-4-11:2004 (Single Phase) IEC61000-4-13:2009 (Single Phase) IEC61000-4-14:1999 (Single Phase) IEC61000-4-17:2009 (Single Phase) IEC61000-4-28:2000 (Single Phase) †IEC61000-4-29:2001 (Single Phase)	IEC61000-3-2:2014 (Single/Three Phase) IEC61000-3-3:2013 (Single/Three Phase) IEC61000-3-12:2005 (Single/Three Phase) IEC61000-3-11:2000 (Single/Three Phase) IEC61000-4-11:2004 (Single/Three Phase) IEC61000-4-13:2009 (Single/Three Phase) IEC61000-4-14:1999 (Single/Three Phase) IEC61000-4-17:2009 (Single Phase) IEC61000-4-28:2000 (Single/Three Phase) †IEC61000-4-29:2001 (Single Phase)	IEC61000-3-2:2014 (Single/Three Phase) IEC61000-3-3:2013 (Single/Three Phase) IEC61000-3-12:2005 (Single/Three Phase) IEC61000-3-11:2000 (Single/Three Phase) IEC61000-4-11:2004 (Single/Three Phase) IEC61000-4-13:2009 (Single/Three Phase) IEC61000-4-14:1999 (Single/Three Phase) IEC61000-4-17:2009 (Single Phase) IEC61000-4-28:2000 (Single/Three Phase) †IEC61000-4-29:2001 (Single Phase)
Measurement Standards	IEC61000-4-7 IEC61000-4-15	IEC61000-4-7 IEC61000-4-15	IEC61000-4-7 IEC61000-4-15
Output Power	6kVA	18kVA	67kVA
Software Included	IECSOFT IEC61000 Test Suite		
Accreditation	Optional UKAS ISO17025 IEC61000 Harmonics and Flicker Certification of PPA5511	Optional UKAS ISO17025 IEC61000 Harmonics and Flicker Certification of PPA5531	Optional UKAS ISO17025 IEC61000 Harmonics and Flicker Certification of PPA5531
Power Measurement Parameters	W, VA, Var, pf, V & A - rms, rectified mean, AC, DC, Peak, Surge, Crest Factor, Form Factor, Star to Delta Voltage Frequency (Hz), Phase (deg), Fundamentals, Impedance Harmonics, THD, TIF, THF, TRD, TDD Integrated Values, Datalog, Sum and Neutral values		
Impedance Network	IMP161 Single Phase 16A Impedance Network	IMP163 Three Phase 16A Impedance Network	IMP753 Three Phase 75A Impedance Network
Current Transformers and Interface	N/A	N/A	3 x LEM IT200-S CT 3 x LEM-1 Interface 1 x LEM-1 PSU
ISO17025 UKAS Certification	Optional - Power Analyzer Calibration	Optional - Power Analyzer Calibration	Optional - Power Analyzer Calibration
Integration of Equipment	Analyzer + Impedance Network fully integrated into rack system		

All specifications at 23°C ± 5°C . These specifications are quoted in good faith but Newtons4th Ltd reserves the right to amend any specification at any time without notice

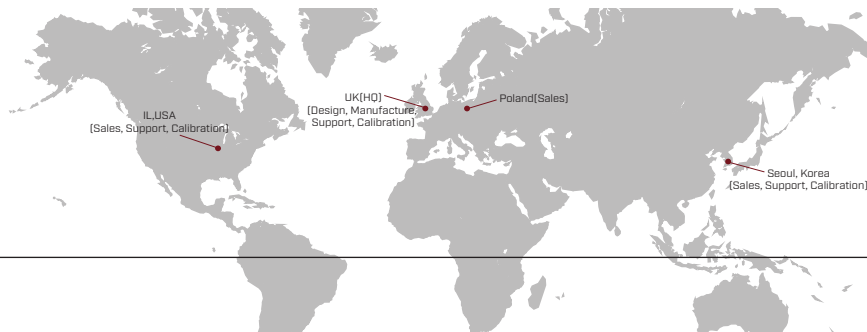

Newtons4th

Newtons4th Ltd (abbreviated to N4L) was established in 1997 to design, manufacture and support innovative electronic equipment to a worldwide market, specialising in sophisticated test equipment particularly related to phase measurement. The company was founded on the principle of using the latest technology and sophisticated analysis techniques in order to provide our customers with accurate, easy to use instruments at a lower price than has been traditionally associated with these types of measurements

Flexibility in our products and an attitude to providing the solutions that our customers really want has allowed us to develop many innovative functions in our ever increasing product range

Contact your local N4L Distributor for further details



THE QUEEN'S AWARDS
FOR ENTERPRISE:
INNOVATION
2010



7949



N4L Newtons4th Ltd

Distributed By :

Newtons4th Ltd 1 Bede Island Road Leicester LE2 7EA UK

Phone: +44 (0)116 230 1066 Fax: +44 (0)116 230 1061
Email: sales@newtons4th.com Web: www.newtons4th.com